



Crit-Line® technology provides caregivers with information about changes in intravascular blood volume and vascular refill rate during dialysis in order to make timely interventions.

## **CLiC™** Device Features

### **Continuous Monitoring of:**

#### Percent Change in Intravascular Blood Volume


Allows the clinician to remove the maximum amount of fluid while preventing common symptoms of dialysis (i.e., nausea, cramping, and vomiting).

### Oxygen Saturation

Provides continuous, accurate measurement of oxygen saturation.

#### Hematocrit and Hemoglobin

Regular monitoring of hematocrit and hemoglobin is important for managing anemia in hemodialysis patients. The CLiC device allows regular, real-time monitoring of hematocrit and calculation of hemoglobin levels during hemodialysis.

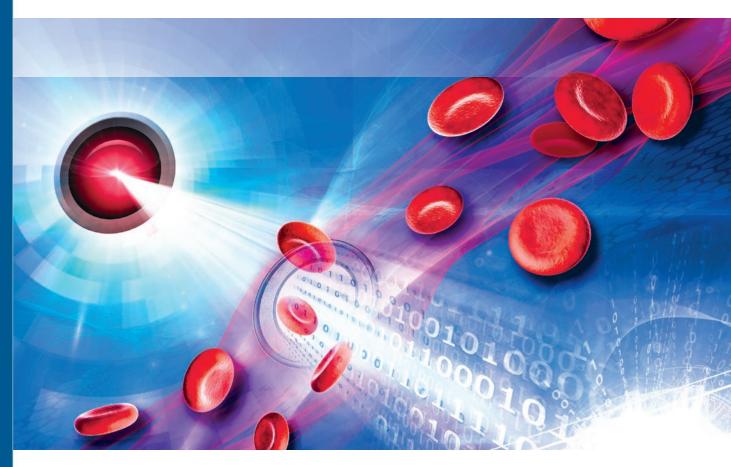



# **Specifications**

Storage and Operating Conditions . . . . . . . . . . . . . 50°F – 104°F (10°C – 40°C)

Transportation Conditions . . . . . . . . . . . . . . . . Avoid extreme temperatures

<-40°F and >257°F (<-40°C and >125°C)

Oxygen Saturation Instrument

Hematocrit Instrument Range & Accuracy . . . . . . . 10 Hct – 60 Hct: ± 1 Hct SD

Ingress Protection IPX0 (CLiC device) IPX1

(2008T hemodialysis machine)

Anesthetic Suitability . . . . . . . . . . . . . . . Not suitable

Modes of Operation . . . . . . . . . . . . . . . . Continuous or Standby

Note: The CLiC device is a Clinical Laboratory Improvement Amendment (CLIA) exempt instrumentation device.



**RENAL TECHNOLOGIES** 

Fresenius Renal Technologies, a division of Fresenius Medical Care North America 920 Winter Street • Waltham, MA 02451 • www.fmcna-crit-line.com

Customer Service: 800-323-5188 • Technical Support: 800-227-2572

Indications for Use: The CLiC device is used with the 2008T hemodialysis machine to non-invasively measure hematocrit, oxygen saturation and percent change in blood volume. The CLiC device measures hematocrit, percent change in blood volume and oxygen saturation in real time for application in the treatment of dialysis patients with the intended purpose of providing a more effective treatment for both the dialysis patient and the clinician. Based on the data that the monitor provides, the clinician/nurse, under physician direction, intervenes (i.e., increases or decreases the rate at which fluid is removed from the blood) in order to remove the maximum amount of fluid from the dialysis patient without the patient experiencing the common complications of dialysis which include nausea, cramping and vomiting. The CLiC blood chamber is a sterile, single use, disposable, optical cuvette designed for use with the CLiC monitor's sensor clip during acute and chronic hemodialysis therapy to non-invasively measure hematocrit, percent change in blood volume and oxygen saturation. The blood chamber is connected between the arterial bloodline and the dialyzer within the extracorporeal circuit during the hemodialysis treatment. The 2008T hemodialysis machine is indicated for acute and chronic dialysis therapy.

Caution: Federal (US) law restricts this device to sale by or on the order of a physician.

**Note:** Read the Instructions for Use for safe and proper use of this device. For a complete description of hazards, contraindications, side effects and precautions, see full package labeling at www.fmcna.com.

© 2014, 2015 Fresenius Medical Care, All Rights Reserved. Fresenius Medical Care, Fresenius Renal Technologies, the triangle logo, 2008, Crit-Line and CLiC are trademarks of Fresenius Medical Care Holdings, Inc., and/or its affiliated companies. All other trademarks are the property of their respective owners.

P/N 102271-01 Rev B 10/2015